



Professional design of
McCormick, Biedseye
View.

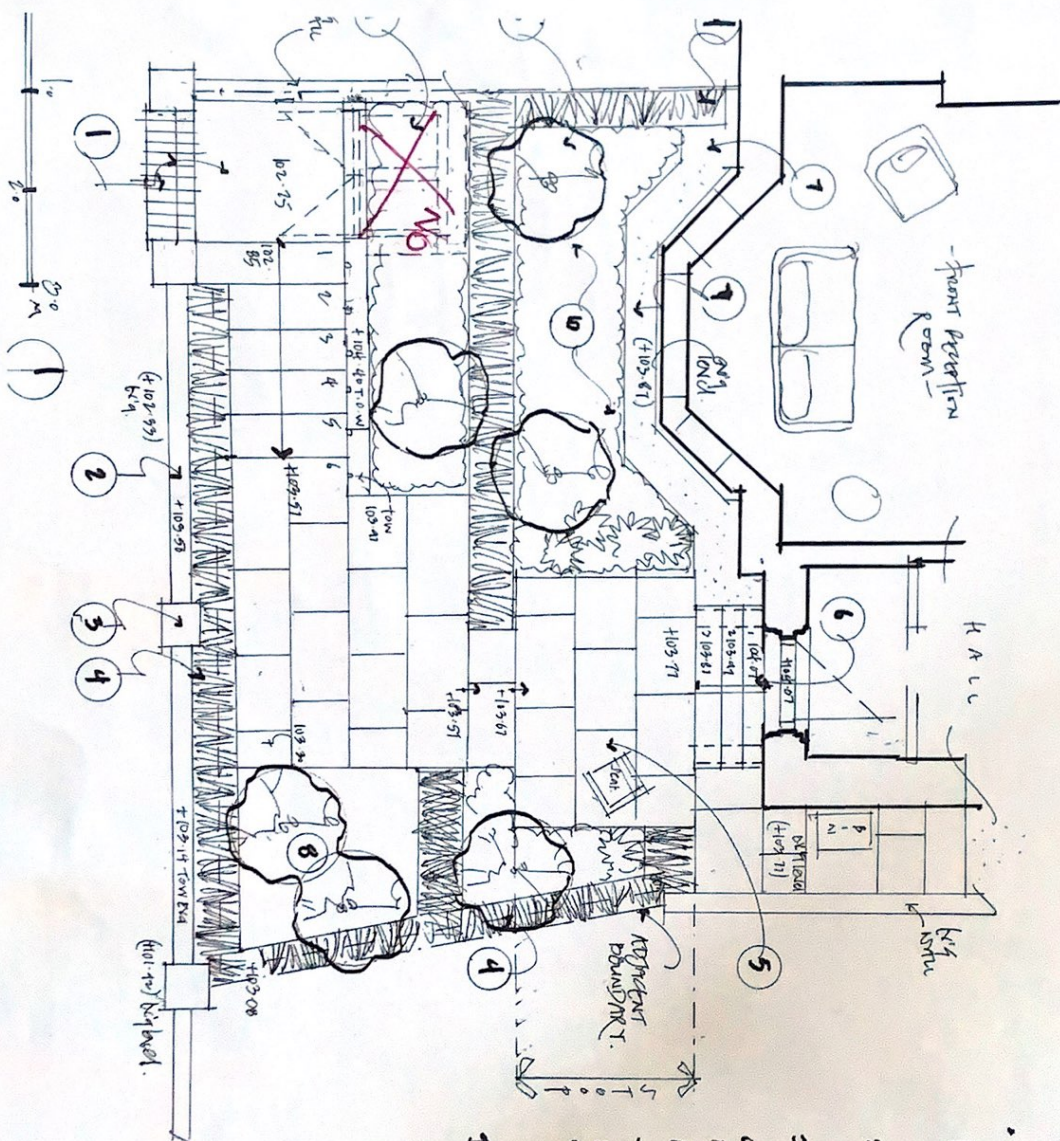

• ONPND •

- 1: Fluerequance i backter and stone influ w/ 6mls from PUDs is accessed w/ 4ths
- 2: Ex i w/ linal performed w/ 2mls covered of pelvic floor to remove w/ linal and coping
- 3: Ex i w/ linal placed to within 100mm of distal spine
- 4: 600mm Yes Hodge
- 5: Stone stop (unusable)
- 6: compressed "fluff" of stone w/ 4ths
- 7: 4th w/ linal removed.
- 8: Fertile w/ 4ths
- 9: Reduced to 100mm at 100mm, Ex i w/ linal placed to 100mm and 100mm w/ 4ths placed to 100mm w/ 4ths
- 10: 100mm ground can be put in w/ 4ths

SECTION OF
BIN STOP

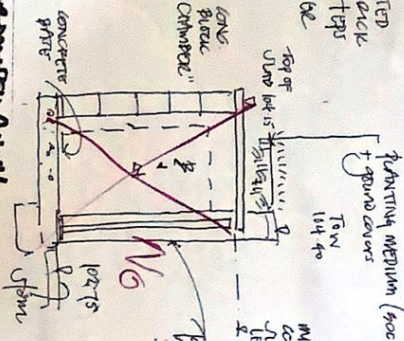

FRONT IMPROVED, WORKMANSHIP ALLEYS

Penicillin concept after 1941

1:30 UST: 2001/2/01